
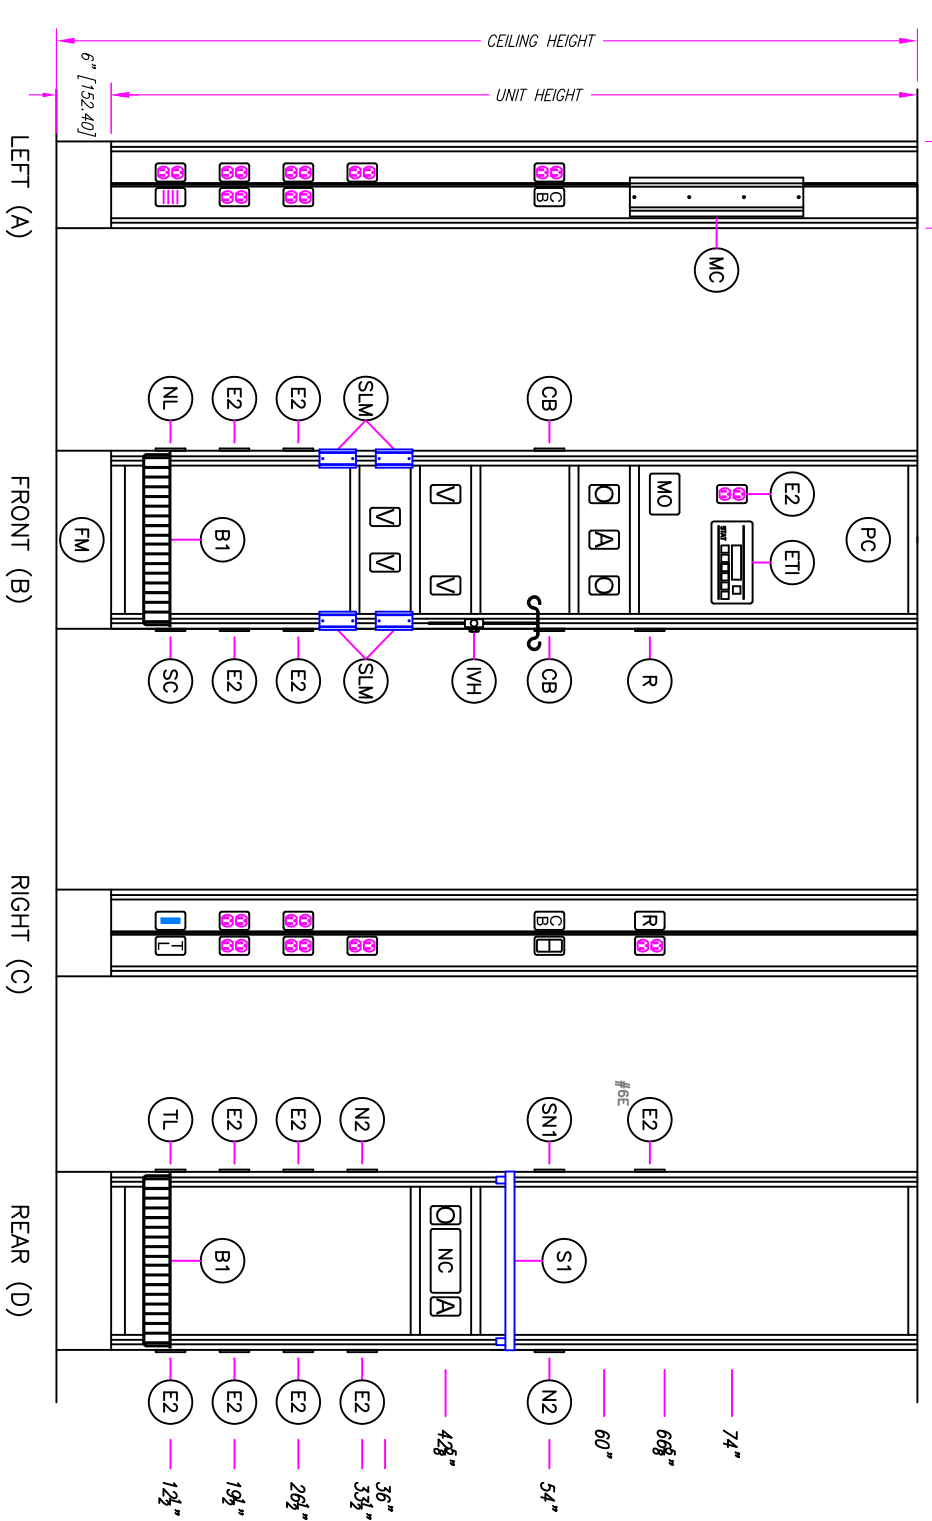


REGAL SERIES 19" POWER COLUMN

FULL LENGTH

(M/N: PC19FL-ICU)

DRAWING # 28

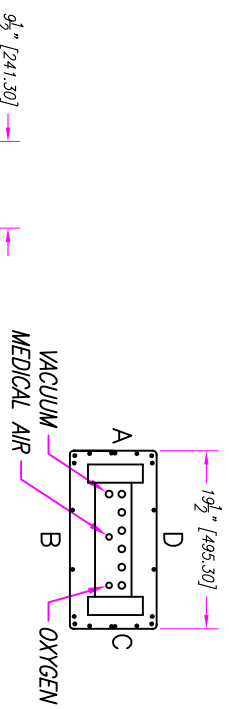

TYPE: _____
 QUANTITY: _____

SYSTEM DETAILS

SYMBOL	QTY.	DESCRIPTION
PC	1	POWER COLUMN, 19"x9"
FM	1	FLOOR MOUNTED SS BASE
VT	8	VERTICAL EQUIPMENT TRACK
O	3	GAS, OXYGEN
A	2	GAS, MED AIR
V	4	GAS, VACUUM
E2	12	RECEPTACLE - DUPLEX RED
N2	2	RECEPTACLE - DUPLEX IVORY
SN1	1	SWITCH, S.P.S.T
NC	1	PROVISION - NURSE CALL 3G
CB	2	PROVISION - CODE BLUE 1G
TL	1	PROVISION - TELEPHONE 1G
MO	1	PROVISION - MONITOR OUT 2G
NL	1	NIGHT LIGHT
SC	1	37 PIN CONNECTOR
SLM	4	VACUUM SLIDE TRACK MTD.
MC	1	MONITOR CHANNEL, MOUNTED
ETI	1	ELAPSED TIME INDICATOR
R	1	E.T.I. RESET
I/H	1	I.V. HOOK - TRACK MTD.
S1	1	SHELF - 20"x12" TRACK MTD.
B1	2	BASKET - 19"x5"x3" TRACK MTD

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE _____

DATE _____ PHONE NO. _____



AMICO Corporation
 85 Fulton Hwy, Ontario
 Richmond Hill, CANADA
 L4B 2N4, CANADA
 Tel: (905) 877-462-6428(F)
 Toll-Free: 1-877-462-6428(F)
 Fax: (905) 764-0800
 Fax: (905) 764-0882
 www.amico.com

HOSPITAL LOCATION: _____
 HOSPITAL LOCATION: _____
 QTY: _____ TYPE: _____ UNITS AS SHOWN / () TYPE: _____ UNITS OPPOSITE

A. NURSE CALL MFR: _____ MODEL NO.: _____
 B. MEDICAL GAS MFR: _____ TYPE CONNECTION: _____
 C. FINISH: _____ CEILING HEIGHT: _____
 DRWG. NO. PRJ3900K-31
 DRAWN BY: _____
 CHECKED BY: _____
 REV. NO.: _____
 DATE: _____