

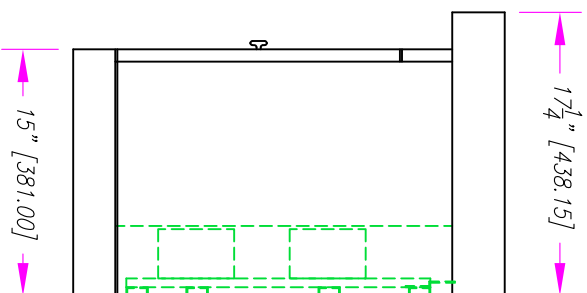
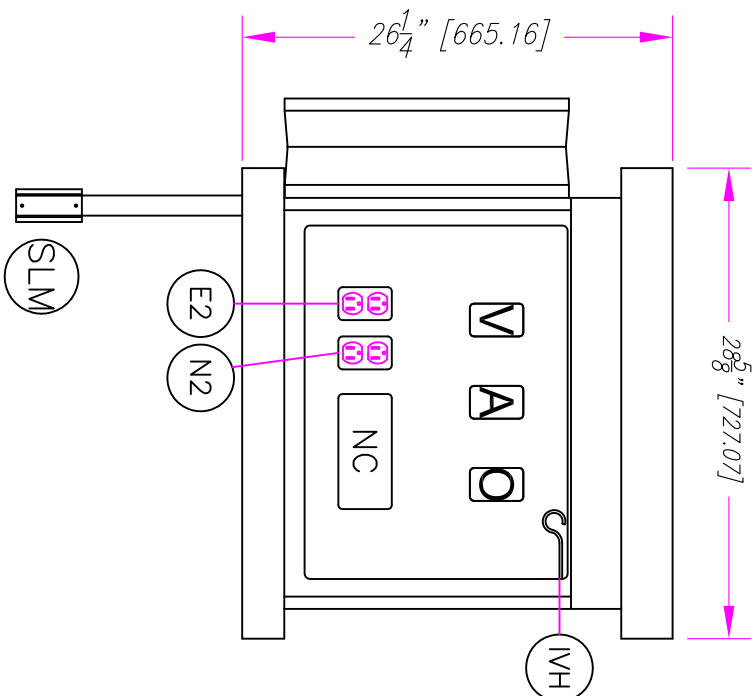


REFLECTION SERIES BABY LDR (M/N: W-REF-ELE-LDRSM)

DRAWING # 53

TYPE:
QUANTITY:

SYSTEM DETAILS	
SYMBOL	DESCRIPTION
O	GAS, OXYGEN
A	GAS, MED AIR
V	GAS, VACUUM
E2	RECEPTACLE - DUPLEX RED
N2	RECEPTACLE - DUPLEX IVORY
NC	PROVISION - NURSE CALL 3G
SLM	VACUUM SLIDE, MOUNTED
IVH	I.V. HOOK, MOUNTED

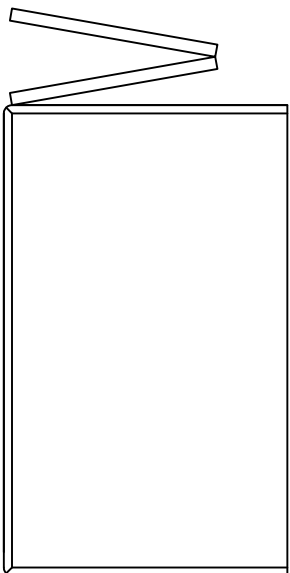

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.

APPROVAL - PRINT AND SIGNATURE _____

DATE _____

PHONE NO. _____

AMICO Corporation
 85 Fulton Hwy,
 Richmond Hill, Ontario
 L4B 2N4, CANADA
 Toll-Free: 1-877-462-6428 (T)
 Tel: (905) 764-0800
 Fax: (905) 764-0882
 www.amico.com

HOSPITAL	HOSPITAL
LOCATION	LOCATION
QTY: 1	() TYPE _____ UNITS AS SHOWN / () TYPE _____ UNITS OPPOSITE

A. NURSE CALL MFGR: _____	MODEL NO.: _____	DRWG. NO. PRICEBOOK-57
B. MEDICAL GAS MFGR.: _____	TYPE CONNECTION: _____	DRAWN BY: _____
C. FINISH: _____	CEILING HEIGHT: _____	CHECKED BY: _____
		REV. NO.: _____
		DATE: _____