SPECTRA SERIES MEDICAL PENDANT

NO.	QTY.	DESCRIPTION
1	1	ANCHOR PLATE (UAP)
2	2	CEILING BEARING
3	1	CEILING COVER
4	4	ARM
5	2	ADAPTER BEARING
6	2	CONSOLE BEARING
7	1	C40 CONSOLE
8	1	C20 CONSOLE

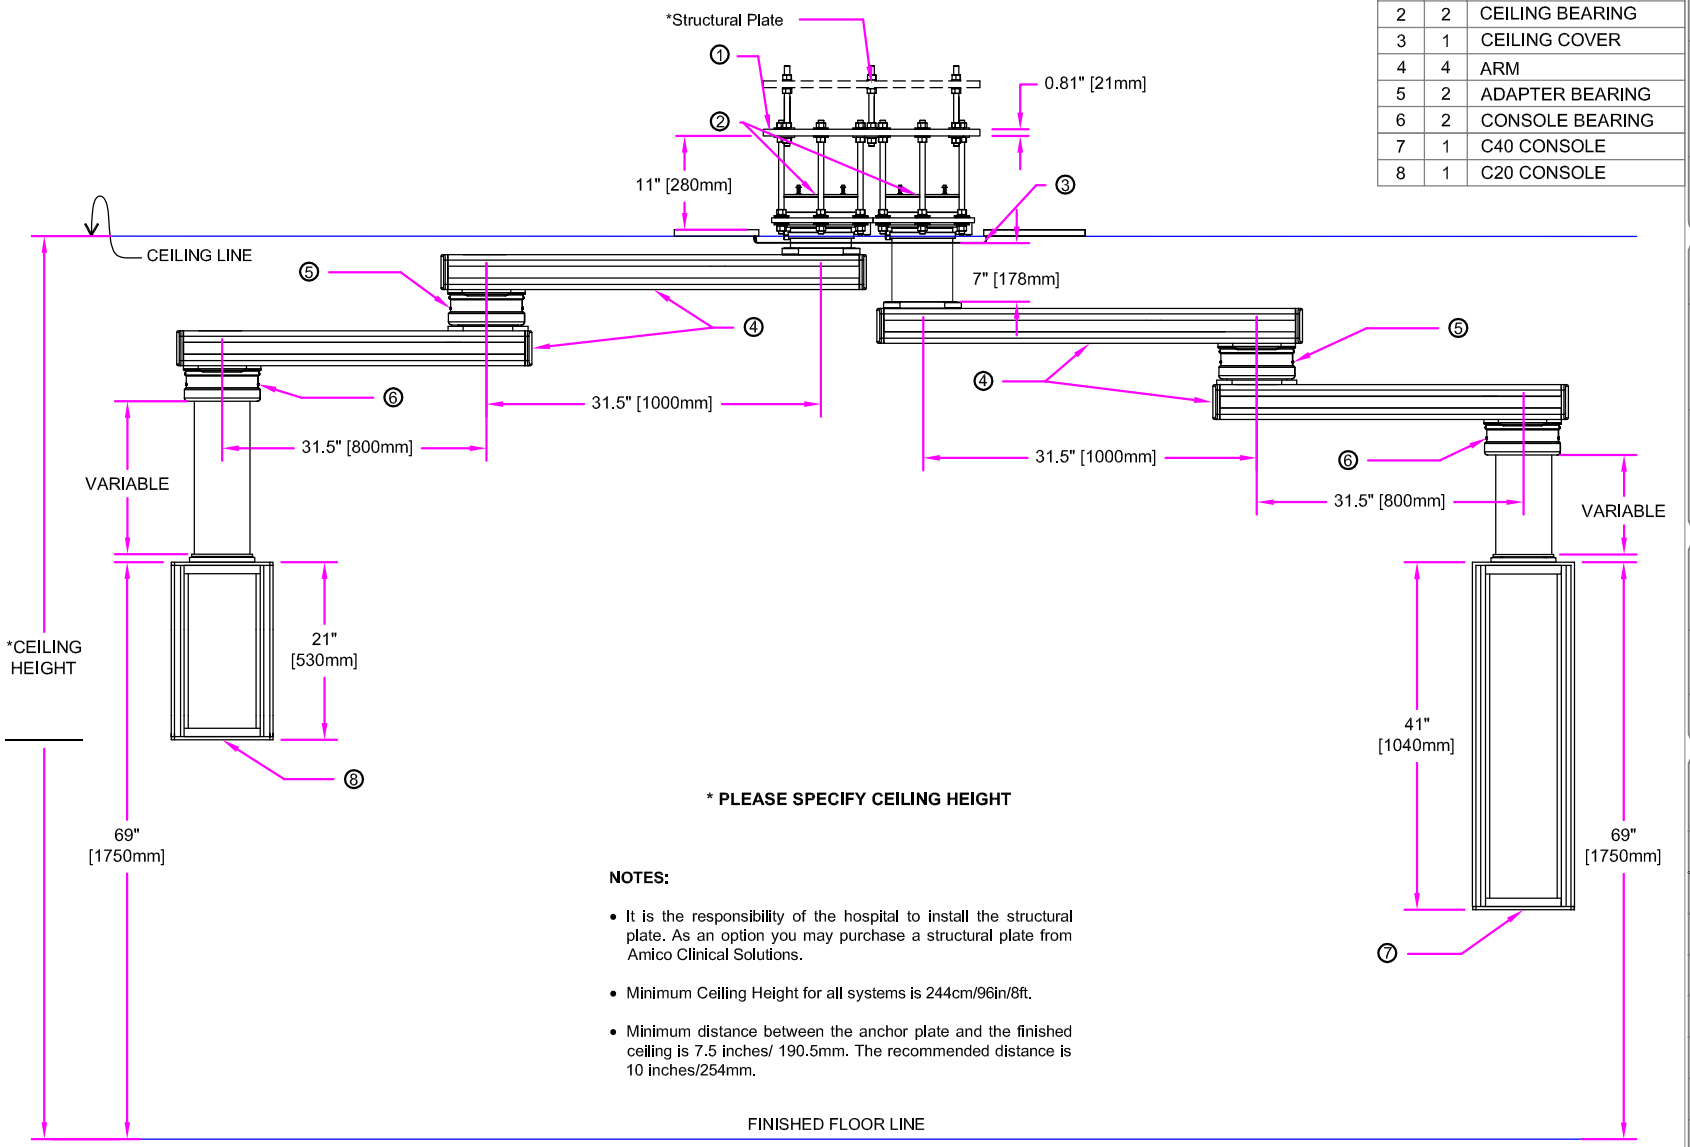

*** PLEASE SPECIFY CEILING HEIGHT**

NOTES:

- It is the responsibility of the hospital to install the structural plate. As an option you may purchase a structural plate from Amico Clinical Solutions.
- Minimum Ceiling Height for all systems is 244cm/96in/8ft.
- Minimum distance between the anchor plate and the finished ceiling is 7.5 inches/ 190.5mm. The recommended distance is 10 inches/254mm.

IMPORTANT: *PLEASE VERIFY THAT THE ABOVE INFORMATION IS CORRECT, AND PROVIDE THE REMAINING DETAILS.*

Amico Clinical
85 Fulton Way
Richmond Hill, ON
L4B 2N4 Canada
Direct Tel: 905-764-0800
Tel: 1-877-462-6426
Fax: 1-866-440-4986
www.amico-clinical.com

TYPE	MAX PAYLOAD EACH ARM	REACH	ROTATION	WEIGHT	BRAKES
DUAL MOUNT - DUAL ARM	654 lbs 297 kg 566 lbs 257 kg	71 " 1800 mm	340°	792 lbs 359 kg	Air / N_2 90 PSI
MODEL: LP-L-1818-N					

PROJECT: LOCATION

ROOM TYPE: ROOM TYPE

OF UNITS:

DATE:

PHONE NUMBER:

APPROVAL SIGNATURE:

DRAWING NUMBER-FILE NAME: MMDDYY-##

DATE: MM/DD/YY | PAGE #: ## OF ##

DRAWN BY: | CHECKED BY:

REV	DATE	DESCRIPTION

DRAWING NOT TO BE USED FOR CONSTRUCTION

THIS DRAWING IS THE PROPERTY OF AMICO CLINICAL. THE INFORMATION CONTAINED HEREIN MAY NOT BE REPRODUCED OR COMMUNICATED TO THIRD PARTIES WITHOUT PRIOR WRITTEN CONSENT