

## DISS



### Features:

- Flow rate exceeds the requirements of NFPA and CSA
- Accepts DISS gas specific adapters
- 100% pressure testing of each outlet and cleaned for medical gas service
- Indexed to eliminate interchangeability of gas services
- Up to 3/4" [19 mm] mounting plate thickness adjustment
- Universal rough-in assembly to accept Quick Disconnects or DISS Front Adapters (can be interchanged at any time)
- Outlets are also available for M.R.I. use
- DISS back body connection

### General Specifications:

The medical gas outlet shall be an Amico Alert-1 series.

Outlet back bodies shall be manufactured with a DISS gas specific fitting which accepts only DISS specific adapters. Body shall be 1-5/16" [33 mm] diameter one piece brass construction.

Outlet bodies shall be gas specific by indexing each gas service to a gas specific dual pin indexing arrangement on the respective identification module.

All M.R.I. outlets are manufactured from nonferrous material.

All outlets shall be cleaned and degreased for medical gas service, factory assembled and tested.

Outlets are UL Listed and ETL Listed.

Amico products comply with NFPA 99 and CSA Z7396.1.


### Project

---

---

---

# Technical Specifications

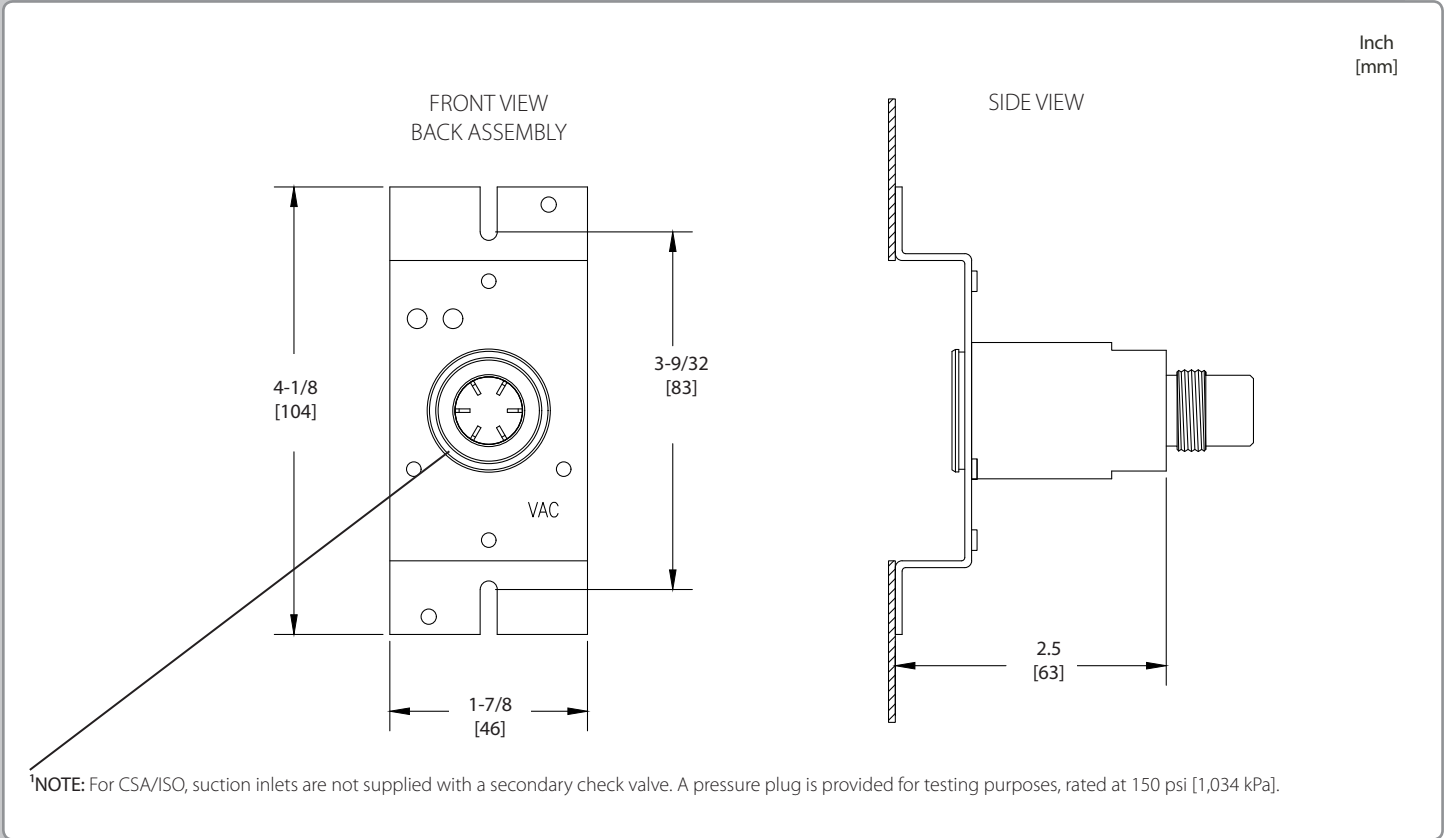

## Model Numbers

**O-BAKCCOD-L-XXX**

**The "L" Defines the Language:**

English (NFPA) Oxy, Air, Vac and WAG only = U  
English (CSA/ISO) = E

**The "XXX" Defines the Gas:**

Oxygen	=	OXY
Medical Air	=	AIR
Nitrous Oxide	=	N2O
Nitrogen	=	NIT
Carbon Dioxide	=	CO2
MedVac <sup>1</sup>	=	VAC
Waste Anesthetic Gas Disposal (NFPA)	=	WAG
Anesthetic Gas Scavenging System <sup>1</sup> (CSA)	=	AGS
Instrument Air	=	INAIR
Heliox	=	HOX

<sup>1</sup>Please see note above

**Distributed By:**



Example: NFPA - DISS, Oxygen = O-BAKCCOD-U-OXY